



# Measurement of methane, nitrous oxide and ammonia in atmosphere with a compact quartz-enhanced photoacoustic sensor

Giansergio Menduni<sup>a</sup>, Andrea Zifarelli<sup>a</sup>, Elena Kniazeva<sup>a</sup>, Stefano Dello Russo<sup>b</sup>,  
Ada Cristina Ranieri<sup>a,c</sup>, Ezio Ranieri<sup>d</sup>, Pietro Patimisco<sup>a</sup>, Angelo Sampaolo<sup>a</sup>, Marilena Giglio<sup>a</sup>,  
Fabrizio Manassero<sup>e</sup>, Elio Dinuccio<sup>f</sup>, Giorgio Provolò<sup>g</sup>, Hongpeng Wu<sup>h</sup>, Dong Lei<sup>h</sup>,  
Vincenzo Spagnolo<sup>a,h,\*</sup>

<sup>a</sup> PolySense Lab - Dipartimento Interateneo di Fisica, Politecnico and University of Bari, Via Amendola 173, Bari, Italy

<sup>b</sup> Italian Space Agency (ASI), Centro di geodesia Spaziale "Giuseppe Colombo", Matera, Italy

<sup>c</sup> Faculty of Engineering, Uninettuno University, 00186 Rome, Italy

<sup>d</sup> Dipartimento di Biologia, Università degli Studi di Bari, Via Orabona 4, 70126 Bari, Italy

<sup>e</sup> ETG Risorse e Tecnologie Srl, Via Padre Carpignano 23, Montiglio Monferrato, Asti, Italy

<sup>f</sup> Department of Agriculture, Forest and Food Science - Div. Agro-Forestry and Environmental Engineering - University of Turin, Largo Paolo Braccini 2, Grugliasco 10095, TO, Italy

<sup>g</sup> Department of Agricultural and Environmental Sciences, Production, Landscape, Agroenergy, University of Milan, Via Celoria 2, Milano 20133, Italy

<sup>h</sup> State Key Laboratory of Quantum Optics and Quantum Optics Devices, Institute of Laser Spectroscopy, Shanxi University, Taiyuan 030006, China

## ARTICLE INFO

### Keywords:

Quartz-enhanced photoacoustic spectroscopy  
Trace gas sensing  
Methane  
Nitrous oxide  
Ammonia  
Multi-gas detection

## ABSTRACT

We demonstrated a 19-inches 6U-rack sensing system based on quartz-enhanced photoacoustic spectroscopy for simultaneous detection of methane, nitrous oxide, and ammonia in atmosphere. The system embeds two detection modules, each one equipped with a quantum cascade laser as light source and a spectrophone composed of a T-shaped quartz tuning fork coupled with acoustic resonator tubes. The sensing system results compact, lightweight, and portable, with a computer interface for an easy end-user operation. The calibration was performed in laboratory environment with certified concentrations. Because of the NH<sub>3</sub> large and permanent dipole moment, ammonia QEPAS signal was used to model and characterize adsorption/desorption processes, for an accurate and reliable sensor calibration. At 0.1 s signal integration time, detection limits of 28 ppb, 9 ppb, and 6 ppb were obtained for CH<sub>4</sub>, N<sub>2</sub>O, and NH<sub>3</sub>, respectively. Since these detection limits were well below the natural abundance of the three analytes in atmosphere, the sensor was employed to monitor CH<sub>4</sub>, N<sub>2</sub>O, and NH<sub>3</sub> concentrations in laboratory air.

## 1. Introduction

With an increasing human population, and the consequent need for more food production, a major challenge for agriculture is the decrease in the environmental footprint. Indeed, agriculture strongly contributes to global environmental change, mainly through emissions of greenhouse gases (GHG). The GHGs danger is measured by their global warming potential (GWP) that quantifies the heat trapping potential of each GHG relative to that of carbon dioxide. Methane (CH<sub>4</sub>) and nitrous oxide (N<sub>2</sub>O) are the most important non-CO<sub>2</sub> GHGs emitted and are characterized by GWPs 28 and 265 times higher than CO<sub>2</sub>, respectively [1–3]. Both pollutants predominantly come from enteric fermentation

produced in the natural part of digestive systems of ruminants, anaerobic decomposition of organic matter in paddy fields emitted by rice cultivation, application and storage of manure and burning of biomass vegetation and crop residues [4,5]. Furthermore, the use of animal manure and nitrogen fertilizers in grain crops production increase the emission of ammonia (NH<sub>3</sub>), contributing to the formation of fine particulate matter, which is considered a major public health concern [6]. Gaseous ammonia has a relatively short lifetime in the atmosphere ranging from a few hours to a few days [7] and is deposited quite close to its source [8]. Typical levels of ammonia can range from concentrations lower than part-per-billion (ppb), up to several part-per-million (ppm) near animal waste lagoons and animal buildings [9]. Accordingly, the

\* Corresponding author at: PolySense Lab - Dipartimento Interateneo di Fisica, Politecnico and University of Bari, Via Amendola 173, Bari, Italy.

E-mail address: [vincenzoluigi.spagnolo@poliba.it](mailto:vincenzoluigi.spagnolo@poliba.it) (V. Spagnolo).

<https://doi.org/10.1016/j.snb.2022.132953>

Received 12 August 2022; Received in revised form 31 October 2022; Accepted 1 November 2022

Available online 3 November 2022

0925-4005/© 2022 The Author(s). Published by Elsevier B.V. This is an open access article under the CC BY-NC-ND license (<http://creativecommons.org/licenses/by-nc-nd/4.0/>).

detection of traces of ammonia in the atmosphere is of interest from both an environmental and a physical point of view.

With the aim to better understand the global warming and the impact on the environment, highly precise and sensitive gas sensors are necessary to determine the source and concentration levels of  $\text{CH}_4$ ,  $\text{N}_2\text{O}$  and  $\text{NH}_3$ . To fulfill the above requirements, optical techniques based on tunable diode laser absorption spectroscopy are the most appropriate methods [10]. Highly performant mid-infrared absorption spectrometers for high precision measurements use quantum cascade lasers (QCLs) as light source to target absorption lines of fundamental bands, with optical powers of several tens of milliwatt. The compactness and the robustness that confer the possibility of a sensor to be employed for in-field operation are determined by the employed gas cell and the capability to preserve over long times the optical alignment between the laser beam and the gas cell. The two types of gas cell that guarantee high stability are the multipass cell and the photoacoustic cell. Multipass cells trap laser beam into multiple reflections between two large diameter focusing mirrors. Optical pathlengths as high as 50 m can be reached with gas cell lengths of few tens of centimeters [11]. Many robust portable sensors employing multipass cells and expensive fast infrared detectors were demonstrated and developed over the last years [12,13]. By squeezing the cell, the effective pathlength is reduced, making impossible to realize efficient multipass cells with physical size of less than 10 cm. Photoacoustic cells are acoustic resonators that amplify the weak sound waves generated by photoacoustic effect occurring within an absorbing gas. The optical alignment is easy, and a microphone is placed at the antinode point of the amplified acoustic pattern within the cell [14]. For Helmholtz acoustic resonators, a normal acoustic mode of few kHz imposes sizes of 10–20 cm for the gas cell. Moreover, the use of microphone requires a rigid acoustic isolation for the external ambient noise. Starting from 2002, an alternative to traditional microphones is represented by quartz tuning forks (QTF) which operate as sharply resonant acoustic transducers [15,16]. This variant of the photoacoustic spectroscopy is named as Quartz-Enhanced Photoacoustic Spectroscopy (QEPAS). The QTF is placed within the gas cell, and it is coupled with a pair of millimeter-size resonator tubes acting as organ pipes. As a result, the gas cell only serves to separate the sample to be analyzed from the external ambient, allowing volumes of few cubic centimeters [17], thus removing restrictions imposed on the gas cell size by the acoustic resonance conditions [18,19]. The laser beam passes through the resonator tubes, between the prongs of the QTF, and is modulated at the QTF resonance frequency or at one of its subharmonics. Due to photoacoustic effect, the sound wave generated between the prongs of the QTF puts them into vibration: the prongs' mechanical deflection is converted into


an electrical signal thanks to the piezoelectricity of the quartz [20]. Thus, QEPAS can face up to requirements to perform reliable measurements of different gases through a modular assembly of centimeter-sizes multiple detection modules into one portable system.

Here we report on the realization of a compact sensing system composed of two QEPAS sensor-heads (SHs). Each sensor-head contains the laser source and a spectrophone composed by a quartz tuning fork resonant at 12.4 kHz and a pair of acoustic resonator tubes. One sensor-head targets two adjacent but not superimposed spectral lines of  $\text{CH}_4$  and  $\text{N}_2\text{O}$  centered at  $1275.04\text{ cm}^{-1}$  and  $1275.49\text{ cm}^{-1}$  respectively, while the other one aims at a  $\text{NH}_3$  absorption line falling at  $1103.44\text{ cm}^{-1}$ . The two sensor-heads were embedded into a compact system equipped with control boards to simultaneously drive both laser sources, as well as to retrieve and analyze the spectrophone signals. It also allows to set the gas pressure and measure its flow.

## 2. Experimental section

The sensor is composed of two sensor-heads with the respective gas lines connected in series, all embedded in a box, as schematically depicted in Fig. 1a. A picture of the final 19-inches 6U-rack sensor system which includes two chemical sensors to also measure  $\text{CO}_2$  and  $\text{H}_2\text{O}$  concentrations, is shown in Fig. 1b.

The optical components of a QEPAS sensor are placed inside the SH, improving the robustness to misalignment, and reducing its overall dimensions. Each SH is composed of a quantum cascade laser (QCL), a ZnSe lens with a focal length of 40 mm, an acoustic detection module (ADM) and an optical power meter (THORLABS PM100USB) for alignment purposes. The ADM (THORLABS ADM01) consists of a spectrophone enclosed in a compact vacuum-tight gas cell equipped with two windows and inlet/outlet gas connectors. The spectrophone is composed of a T-shaped QTF acoustically coupled with a pair of resonator tubes having a length of 12.4 mm and an inner diameter of 1.59 mm. This configuration has proven to provide the highest signal to noise ratio enhancement with respect to the bare QTF [21,22]. For each SH, the collimated laser beam is focused into the ADM, passing through the resonator tubes and between the QTF prongs. When the laser wavelength is modulated and tuned to an absorption feature, the photoacoustic effect occurs, and a standing wave vibrational pattern is created within the spectrophone. SH1 mounts a QCL (Thorlabs QD7840HHLH-A) which targets two adjacent absorption features of  $\text{CH}_4$ , centered at  $1275.04\text{ cm}^{-1}$  and  $1275.39\text{ cm}^{-1}$  with their respective linestrengths of  $3.73 \cdot 10^{-20}\text{ cm/molecule}$  and  $2.48 \cdot 10^{-20}\text{ cm/molecule}$ , and an absorption feature of  $\text{N}_2\text{O}$ , centered at  $1275.49\text{ cm}^{-1}$  with a

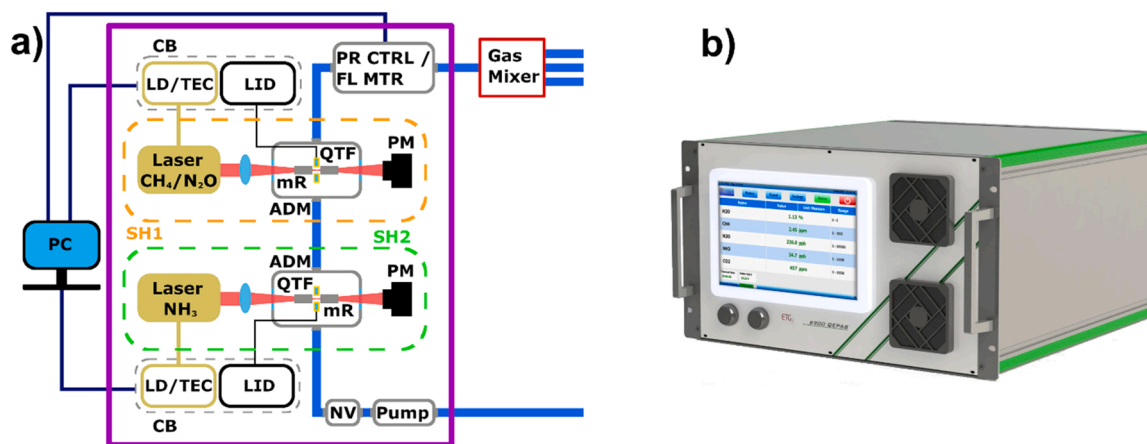

**Fig. 1.** a) Schematic of the sensor box composed of two QEPAS sensor heads, one for detection of  $\text{CH}_4$  and  $\text{N}_2\text{O}$ , the other for  $\text{NH}_3$  detection, connected in series in the same gas line. b) Picture of the realized 19-inches 6U-rack sensor. Size: 35cmx55cmx44cm, weight 14 kg. PC – Personal Computer; QTF – Quartz Tuning Fork; mR – Resonator tubes; ADM – Acoustic Detection Module; PM – Power Meter; SH1 – Sensor Head 1; SH2 – Sensor Head 2; CB – Control Board; LD – Laser Driver; TEC – Thermoelectric Cooler; LID – Lock-In Detection; PR CTRL/FL MTR – Pressure controller/ Flow Meter; NV – Needle Valve.

linestrength of  $1.42 \cdot 10^{-19}$  cm/molecule [23]. In SH2, the laser source is a QCL (Thorlabs QD9062HHLH-C), capable to target the absorption line of  $\text{NH}_3$  at  $1103.44 \text{ cm}^{-1}$ , having a linestrength of  $1.51 \cdot 10^{-19}$  cm/molecule [23]. The QCLs injection currents and temperatures were controlled by the Merstetter Engineering LTC-1141 control boards (CB). For SH1, the QCL temperature was fixed at  $20^\circ\text{C}$  to target the  $1275.04 \text{ cm}^{-1}$   $\text{CH}_4$  line at an injected current of 319 mA with an optical power of 74 mW, and the  $\text{N}_2\text{O}$  line at 340 mA with an optical power of 77 mW. The QCL mounted in the SH2 operates also at  $20^\circ\text{C}$  and the  $\text{NH}_3$  line is targeted with an injection current of 320 mA corresponding to a laser power of 59 mW. In addition, the selected laser driver provides both a slow triangular ramp current modulation to each laser to scan the selected absorption features, and a fast sinusoidal modulation. In this work, QEPAS measurements were performed in wavelength modulation and 2f-detection (WM-2f): for each SH, the laser sinusoidal modulation is set at half of the resonance frequency of its spectrophone, while the response is demodulated at its resonance frequency. The QTF current signals were converted into voltage signals by a transimpedance amplifier, with a  $10 \text{ M}\Omega$  feedback resistor. The selected CB is equipped with an analog input terminal, allowing the acquisition and the on-board processing of the QTF signal. A custom-firmware was developed to detect the 2f-component of the signal, via a lock-in acquisition and the data have been acquired with an integration time of 0.1 s. In the calibration phase of the sensor, the gas delivery system is composed of (i) a gas mixer (MCQ Instrument Gas Blender GB1A30120164) whose output was connected to a Nafion tube to fix the water concentration (not shown in Fig. 1), and in turn to the input valve of the sensor box; (ii) a pressure controller/flow meter (MKS Type 649); (iii) a needle valve; and iv) a vacuum pump (KNF N 813.4). The selected components were employed to stabilize the pressure and fix the gas flow at 50 sccm in the two SHs. Under these conditions, the Nafion humidifier allowed keeping stable the water concentration in all investigated gas mixtures to 1.2 %. The gas mixer was removed from the gas line for atmospheric measurements of the three gases, and the gas sample from outside directly flowed through the Nafion humidifier and then the SHs.

## 2.1. Selection of the pressure working condition

The developed sensor aims at detecting three important environmental gas species, i.e., methane, nitrous oxide, and ammonia. Since the performance of QEPAS sensors depends on the pressure working condition, the pressure dependence of the QEPAS signal was investigated for each target gas and the results are shown in Fig. 2. The amplitude and the frequency of sinusoidal modulation were optimized for each pressure value. For all three gases, certified concentrations mixed with a synthetic standard air matrix (composed by 21 % of  $\text{O}_2$  and 79 % of  $\text{N}_2$ ) were flowed in the gas line.

The methane peak signals measured for a mixture of 50 ppm of  $\text{CH}_4$  in standard air in the 100 – 700 Torr pressure range are shown in Fig. 2a. The highest QEPAS signal was measured at 500 Torr. In the same

pressure range, the  $\text{N}_2\text{O}$  peak signal of a mixture containing 10 ppm of  $\text{N}_2\text{O}$  diluted in standard air was measured and the results are shown in Fig. 2b. The maximum signal was measured at 300 Torr, while a 18 % reduction of the signal was recorded at 500 Torr. For a 14 ppm of  $\text{NH}_3$  diluted in standard air, the SH2 response reaches its maximum value at 500 Torr. Since the two SHs have to be operated at the same pressure, we selected 500 Torr as operating pressure and all reported measurements in next paragraphs have been acquired under this condition. Consequently, the resonance properties of both spectrophones, in terms of resonance frequency and quality factor, were measured at 500 Torr. The SH1 spectrophone shown a resonance frequency of 12,465.0 Hz and a quality factor of 15910, while the SH2 spectrophone resonated at 12,467.6 Hz with a quality factor of 13180.

## 2.2. Methane and nitrous oxide calibration with sensor head 1

For methane and nitrous oxide calibrations, standard air was used to dilute a cylinder with a certified concentration of 10 ppm of  $\text{CH}_4$  in synthetic air and another one with a certified concentration of 10 ppm of  $\text{N}_2\text{O}$  in synthetic air, respectively. The QEPAS spectral scans of the selected  $\text{CH}_4$  absorption lines were acquired in WM-2f by applying a sinusoidal current modulation with a peak-to-peak value of 10 mA. The same current modulation was applied to retrieve the  $\text{N}_2\text{O}$  absorption feature. Figs. 3a and 3b show the QEPAS spectral scans acquired for  $\text{CH}_4$  and  $\text{N}_2\text{O}$  calibrations, respectively, in the 1–10 ppm concentration range.

As expected from the HITRAN database, together with the most intense methane peak in the laser tuning range falling at 36 s, also the  $\text{CH}_4$  peak at  $1275.39 \text{ cm}^{-1}$  is visible at 18 s. Hereafter, only the  $\text{CH}_4$  peak falling at  $1275.04 \text{ cm}^{-1}$  will be considered for the analysis, since it allows higher sensitivity. The methane and nitrous oxide absorption features do not spectrally overlap in the laser tuning range, therefore the peak values of the QEPAS signals can be employed to measure the concentration of each gas in the mixture. The peak values were extracted from each spectral scan in Figs. 3a and 3b and plotted as a function of the related analyte concentration in Figs. 4a and 4b, respectively.

As shown in Fig. 4a-b, the signal of both gases linearly depends on the analyte concentration. The linear fit of the two calibration curves yields a slope of 8.18 mV/ppm and 26.67 mV/ppm which represent the sensitivity for methane and nitrous oxide detection, respectively. The minimum detection limit (MDL) of the sensor was calculated as the ratio between the noise level and the sensitivity. The  $1\sigma$ -noise level was measured as the standard deviation of the acquired data when standard air was flowing through SH1. With a  $1\sigma$ -noise level of 230  $\mu\text{V}$  at an integration time of 0.1 s, MDLs of 28 ppb and 9 ppb can be estimated for methane and nitrous oxide, respectively. The noise level can be lowered by further averaging the signal over longer times. An Allan-Werle deviation analysis was performed with the aim of estimating the  $1\sigma$  noise (and thus the achievable MDL) as a function of the integration time. The laser was locked far from both the absorption features while standard air

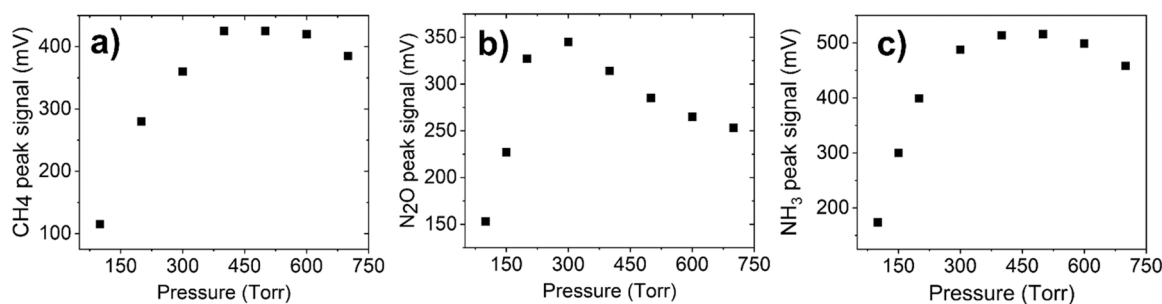


Fig. 2. a)  $\text{CH}_4$  QEPAS signals as a function of the pressure when a mixture of 50 ppm of  $\text{CH}_4$  in standard air flows in the sensor box. b)  $\text{N}_2\text{O}$  QEPAS signal as a function of the pressure for a mixture of 10 ppm of  $\text{N}_2\text{O}$  diluted in standard air. c)  $\text{NH}_3$  QEPAS signal acquired at different pressures for a mixture of 14 ppm of  $\text{NH}_3$  in standard air.

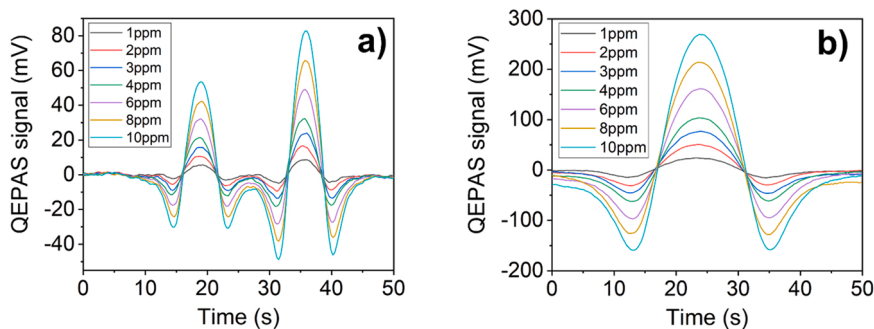


Fig. 3. a) QEPAS spectral scans measured for different  $\text{CH}_4$  in standard air concentrations. b)  $\text{N}_2\text{O}$  QEPAS scans measured for 7 different  $\text{N}_2\text{O}$  concentrations in standard air.

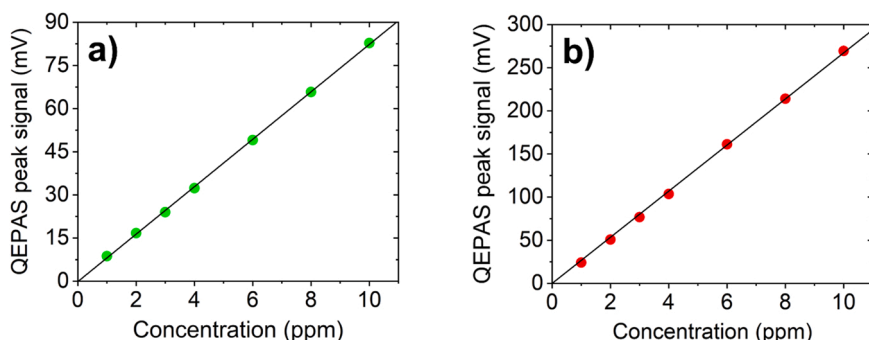


Fig. 4. (a) Peak values measured for each methane concentration (green dots). The black solid line is the best linear fit of the experimental data. (b) QEPAS peak signal as a function of  $\text{N}_2\text{O}$  concentration (red dots) with the corresponding best linear fit (black line).

flows in the SH1. The obtained Allan-Werle deviation plot is reported in Fig. 5.

For an integration time of 10 s the  $1\sigma$ -noise level can be lowered to  $\sim 50 \mu\text{V}$ , corresponding to minimum detection limits of 6 ppb and 2 ppb for  $\text{CH}_4$  and  $\text{N}_2\text{O}$ , respectively. These detection limits can be further improved by increasing the integration up to 30 s. For longer integration times, drift effects emerge, mainly induced by mechanical instabilities which causes a deterioration of the overall sensor head performance.

### 2.3. AMMONIA calibration with sensor head 2

During the transport of a gas through a tube or cell, adsorption effects appear, especially in the case of polar molecules such as ammonia and water. Adsorption or desorption effects result in a change of the gas-phase concentration. Polar molecules such as  $\text{NH}_3$  with large and

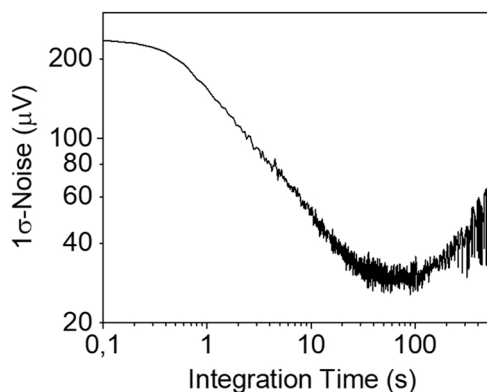


Fig. 5. Allan-Werle deviation plot of the QEPAS signal as a function of the integration time. For a 10 s integration time, the  $1\sigma$ -noise level can be lowered to  $\sim 50 \mu\text{V}$ .

permanent dipole moment have a strong tendency to stick to surfaces. The adsorption/desorption processes depend both on physical properties of the internal surface (material, temperature, porosity) and on experimental conditions (gas flow and analyte concentration) [24]. In this work, the gas delivery system tubing is made of thermoplastic polyurethane (TPU). The internal wall surface of a sensor and tubes can be considered as a place with free binding sites for  $\text{NH}_3$  molecules as well as a reservoir of molecules. Thereby, adsorption/desorption processes need to be considered for accurately determining the concentration of ammonia. With respect to  $\text{NH}_3$ , the  $\text{N}_2\text{O}$  and  $\text{CH}_4$  dipole moment is much lower. For this reason, it is not necessary to consider their adsorption/desorption processes for their reliable calibration [25].

While a mixture is flowing within the sensor, an equilibrium condition can be achieved between the surface coverage and molecules concentration. Therefore, flowing a gas with a known concentration through a cell, the adsorption is quantified in terms of the time needed to reach a steady-state concentration. Conversely, when the gas species is removed from the gas line, molecules released from the reservoir will increase the number of molecules in the gas mixture (desorption process). In both cases, adsorption-desorption processes will negatively affect the accuracy of a gas detection technique.

The dynamic equilibrium between adsorption-desorption processes can be expressed by a qualitative theoretical model in terms of time and spatial derivatives of  $\text{NH}_3$  concentration and surface coverage, i.e., the number of particles per area [26,27]:

$$\frac{\partial c_g(x, t)}{\partial t} = -u \frac{\partial c_g(x, t)}{\partial x} - \frac{dS}{dV} \frac{\partial c_w(x, t)}{\partial t} \quad (1)$$

where  $c_g$  is the ammonia concentration in the gas mixture,  $c_w$  is the ammonia surface coverage,  $dS$  is the infinitesimal surface area,  $dV$  is the infinitesimal volume,  $u$  is the drift velocity of the gas mixture which can be expressed as the ratio between the flow velocity  $\Phi$  and the cross-sectional area  $A$ , and  $x$  is the direction of flow, assumed to be



rectilinear. Since the ammonia concentration is measured at the point  $x = x_{meas}$ , the Eq. 1 can be integrated from the entrance of the sensor system,  $x = 0$ , where the ammonia concentration is  $c_g^0$  to  $x = x_{meas}$  where a concentration  $c_g^m$  is measured, leading to:

$$\frac{\partial c_g^m(t)}{\partial t} = \frac{\Phi}{V} [c_g^0 - c_g^m] - \frac{S}{V} \frac{\partial c_w(x, t)}{\partial t} \quad (2)$$

The factor  $\Phi/V$  is the inverse of the characteristic gas-exchange time  $\tau_0$ .  $\partial c_w / \partial t$  represents the effective adsorption rate, namely the difference between the adsorption rate and the desorption rate.  $\partial c_w / \partial t$  can be expressed in the form of a dynamic exchange of molecules between the surface and the gas by separating the two contributions. If the surface wall coverage saturation is  $c_{w0}$ , the molecules of gas lost to the surface per unit time (adsorption) can be assumed proportional to the density of free binding sites on the surface,  $c_{w0} - c_w$ , while the number leaving the surface per unit time (desorption) is proportional to the density of occupied sites  $c_w$ :

$$\frac{\partial c_w}{\partial t} = k_1 (c_{w0} - c_w) - k_2 c_w \quad (3)$$

where  $k_1$  and  $k_2$  are the proportionality constants. With this formulation, adsorption and desorption can be separated. This allows the identification of two distinguishable situations: i) the sensor contains no ammonia and at a certain time a gas mixture with a fixed ammonia concentration  $c_0$  starts to flow inside (sensor filling); ii) the sensor contains a mixture with fixed concentration of ammonia  $c_0$  and a certain point it is pumped out by flushing standard air (sensor cleaning). It is safe to assume that the desorption is negligible during sensor filling and, conversely, the adsorption can be neglected during the sensor cleaning. For sensor filling, Eq. 3 becomes:

$$\left( \frac{\partial c_w}{\partial t} \right)_f = k_1 (c_{w0} - c_w) \quad (4)$$

which has as solution:

$$c_w(t)|_f = c_{w0} \left( 1 - e^{-\frac{t}{\tau_1}} \right) \quad (5)$$

where  $\tau_1 = 1/k_1$ . By combining Eqs. 2 and 5 and imposing the boundary condition  $c_g^m(0) = 0$  and  $c_g^0 = c_0$ ,  $c_g^m(t)|_f$  can be expressed as:

$$c_g^m(t)|_f = A_0 \left( 1 - e^{-\frac{t}{\tau_0}} \right) + A_1 \left( 1 - e^{-\frac{t}{\tau_1}} \right) \quad (6)$$

where:

$$A_1 = \frac{S \cdot c_{w0}}{\Phi(\tau_1 - \tau_0)} \quad (7)$$

and  $A_0 = c_0 - A_1$ .

For sensor cleaning, the first term of right-hand side of Eq. 3 can be neglected and its solution is:

$$c_w(t)|_c = c_{w0} e^{-\frac{t}{\tau_2}} \quad (8)$$

where  $\tau_2 = 1/k_2$ . Again, by combining Eqs. 2 and 8 and imposing the boundary condition  $c_g^m(0) = c_0$  and  $c_g^0 = 0$ , the  $c_g^m(t)|_c$  can be expressed as:

$$c_g^m(t)|_c = A_2 \left( 1 - e^{-\frac{t}{\tau_0}} \right) - A_3 \left( 1 - e^{-\frac{t}{\tau_2}} \right) \quad (9)$$

with:

$$A_3 = \frac{S \cdot c_{w0}}{\Phi(\tau_2 - \tau_0)} \quad (10)$$

and  $A_2 = c_0 - A_3$ .

To estimate  $\tau_0$ ,  $\tau_1$  and  $\tau_2$ , a mixture of 14 ppm of  $\text{NH}_3$  in standard air

and standard air were used as channel inputs to the gas blender. The situation of sensor filling was realized starting with standard air flowing inside the sensor box: at a certain time (corresponding to  $t = 0$  of the theoretical model) a fast switching interrupts the standard air flows and the mixture of  $\text{NH}_3$  starts to flow. Conversely, the sensor cleaning starts with the mixture of  $\text{NH}_3$  and moves to a fast switch at  $t = 0$  to the standard air. In both cases, the laser current was locked to  $\text{NH}_3$  absorption peak while the sinusoidal modulation is applied with a peak-to-peak current of 15 mA, in WM-2f detection. The  $\text{NH}_3$  QEPAS signal normalized to the unit as a function of time during the filling and cleaning procedure is reported in Figs. 6a and 6b, respectively.

As shown in the inset of Fig. 6a, the initial signal rise has a positive concavity until  $t = 92$  s where there is an inflection point. Thus, for  $t < 92$  s, the QEPAS signal rises more slowly than that predicted by Eq. 6, suggesting the presence of nonlinear effects that are not included in the simplified theoretical model [26]. This initial QEPAS signal behavior can be ascribed to the starting huge density of free binding sites on the sensor inner surfaces, consequently the probability for  $\text{NH}_3$  molecules to be captured is very high and few molecules reach the measurement point, i.e., the spectrophone. When these sites start to be filled, the  $\text{NH}_3$  molecules more easily reach the spectrophone and a dynamic equilibrium between the gas flux and the adsorption processes can be established, which is the condition imposed by the theoretical model during the transient. A similar situation is also observed in the sensor cleaning process: the QEPAS signal decrease looks like delayed until  $t = 60$  s, then the signal drops down with a positive concavity, as predicted by Eq. 9. Based on these considerations, only experimental data beyond the inflection points were fitted by using Eq. 6 and Eq. 9 and reported as solid red line in Fig. 6a and Fig. 6b for the filling and cleaning processes, respectively. The fitting procedure gives  $\tau_0 = 93$  s and  $\tau_1 = 966$  s for the filling procedure and of  $\tau_0 = 107$  s and  $\tau_2 = 1212$  s for the cleaning procedure. In both cases, the time constant related to adsorption/desorption processes is more than one order of magnitude higher than the characteristic gas-exchange time  $\tau_0$ , which is related only to the dimensions of the sensor and the gas flow. These obtained results were employed to accurately calibrate the sensor.


The calibration of SH2 for  $\text{NH}_3$  was performed as for SH1, starting from the certified concentration of 14 ppm of  $\text{NH}_3$  in standard air and mixing it with standard air matrix. For each dilution, a waiting time of 60 min for reaching a steady-state signal was considered. After that, the sensor was cleaned before moving to the next dilution. The QEPAS scans referred to different  $\text{NH}_3$  concentrations in standard air are reported in Fig. 7a.

The peak values are plotted as a function of the  $\text{NH}_3$  concentration in Fig. 7b, together with the linear fit which returns a sensitivity of 37.22 mV/ppm, corresponding to an MDL of 6 ppb ( $1\sigma$ -noise level of 210  $\mu\text{V}$ ) at an integration time of 0.1 s. The Allan-Werle analysis of the  $1\sigma$  noise level is reported in Fig. 8.


The noise level can be lowered to 50  $\mu\text{V}$  when the signal integration time is increased to 10 s and consequently the minimum detection limit reaches 1.4 ppb.

### 3. Measurement of atmospheric ammonia, methane and nitrous oxide


The MDLs reached for the three gas species at an integration time of 0.1 s are below the natural abundance of the three analytes, thus making SH1 and SH2 suitable for the monitoring of their levels in environmental air. The sensor was employed to measure the concentrations of methane, nitrous oxide, and ammonia in laboratory air for more than 4 h. The use of the Nafion humidifier allowed keeping stable the water concentration to 1.2 %. This approximately corresponds to 50 % relative humidity at 20 °C. This setting is reasonable because the relative humidity of the laboratory air is significantly lower than 50 %. For the cases in which the relative humidity is higher than 50 %, one possibility is to insert a membrane gas dryer before the tube humidifier for an upstream

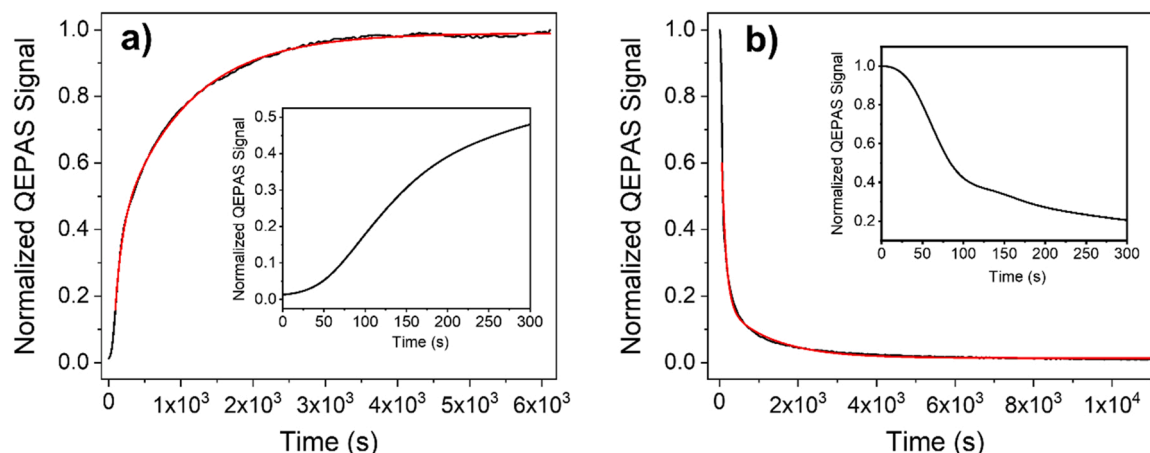

**Fig. 6.** (a) Normalized QEPAS signal as function of time acquired locked on  $\text{NH}_3$  absorption peak during filling step (black curve) together with the performed exponential fit (red curve) based on Eq.6. Inset: zoom on the inflection point observed in the initial signal rise. (b) Normalized QEPAS signal as function of time acquired locked on  $\text{NH}_3$  absorption peak during cleaning step (black curve) together with the performed exponential fit (red curve) based on Eq.9. Inset: zoom on the inflection point observed in the initial signal decrease.

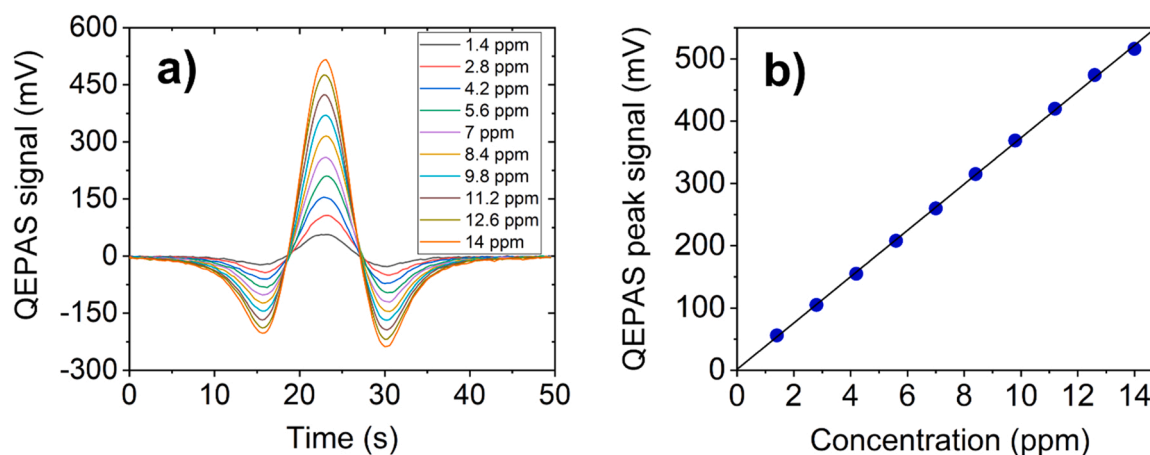


**Fig. 7.** (a) 2f-QEPAS spectra collected by varying the  $\text{NH}_3$  concentration within the gas cell. (b) QEPAS peak signals extracted from spectral scans reported as function of  $\text{NH}_3$  concentration (blue dots). The performed best linear fit is superimposed to the collected data (black line).

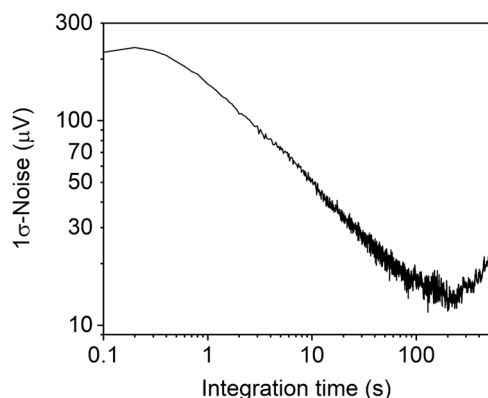

**Fig. 8.** Allan-Werle deviation analysis for  $\text{NH}_3$  sensor. The estimated  $1\sigma$ -noise level is reported as a function of sensor integration time.

reduction of the relative humidity below 50 %. A software was developed to drive both sensor heads and acquire and process the QEPAS signals. The measurements were performed at 500 Torr by acquiring QEPAS spectral scans of the  $\text{CH}_4$  and  $\text{N}_2\text{O}$  absorption lines with SH1 and the QEPAS spectral of the  $\text{NH}_3$  absorption line with SH2, both operating

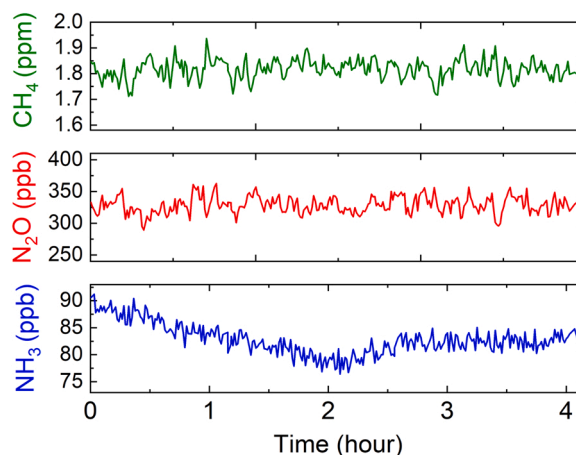

**Fig. 9.** QEPAS peak signals extracted by consecutive QEPAS spectra acquired by sampling the air inside the laboratory at fixed  $\text{H}_2\text{O}$  concentration of 1.2 %. SH1 was used to monitor  $\text{CH}_4$  (green line) and  $\text{N}_2\text{O}$  (red line) concentrations, while sensor SH2 was used to detect  $\text{NH}_3$  (blue line).

at 0.1 s integration time. For each spectral scan, the QEPAS peak signals of CH<sub>4</sub>, N<sub>2</sub>O, and NH<sub>3</sub> absorption features were extracted and are plotted as a function of time in Fig. 9. The time interval between two consecutive peaks of the same analyte was 50 s. The reported concentrations were calculated using the calibration curve of each analyte, reported in Fig. 4a-b and Fig. 7b.

The extracted peaks returned stable concentrations of methane and nitrous oxide, with an average CH<sub>4</sub> concentration of 1.81 ppm, with a standard deviation of 0.04 ppm, and an average N<sub>2</sub>O concentration of 330 ppb, with a standard deviation of 13 ppb. These measured values are consistent with the expected CH<sub>4</sub> and N<sub>2</sub>O levels in atmosphere [28]. The ammonia concentration slightly varied during the measurement period, with an average level of 83 ppb and a standard deviation of 3 ppb. This NH<sub>3</sub> level is coherent with the typical levels of ammonia in indoor air [6].

#### 4. Conclusions

In this work, we reported on a portable QEPAS 19-inches 6U-rack sensor system capable to detect methane, nitrous oxide, and ammonia, three important analytes for the study of the environmental footprint of agriculture and food production industry. The realized QEPAS sensor is composed of two sensor heads, connected in series. The first sensor head is equipped with a QCL, capable to target two adjacent absorption features of CH<sub>4</sub>, centered at 1275.04 cm<sup>-1</sup> and 1275.39 cm<sup>-1</sup>, and an absorption feature of N<sub>2</sub>O, centered at 1275.49 cm<sup>-1</sup>. A QCL capable to detect the NH<sub>3</sub> absorption feature at 1103.44 cm<sup>-1</sup> was selected and mounted in SH2. The same type of spectrophone, composed of a 12 kHz T-shaped QTF coupled with optimized resonator tubes, was employed in both sensor heads. At an integration time of 0.1 s, the CH<sub>4</sub> and N<sub>2</sub>O minimum detection limits were 28 ppb and 9 ppb, respectively. Since ammonia is a polar molecule with large and permanent dipole moment, adsorption/desorption processes were modeled and considered for an accurate calibration of the sensor. An NH<sub>3</sub> minimum detection limit of 6 ppb at an integration time of 0.1 s was obtained, considering a waiting time of 60 min between each concentration in the calibration phase. The sensor was employed to monitor the concentration of CH<sub>4</sub>, N<sub>2</sub>O and NH<sub>3</sub> in laboratory air, since the achieved detection limits were all below the natural abundance of the three gas species in atmosphere. This measurement returned an average CH<sub>4</sub> concentration of 1.81 ppm, an average N<sub>2</sub>O concentration of 330 ppb and an average NH<sub>3</sub> concentration of 83 ppb. These results are compatible with the expected levels of these analytes in indoor air. Considering the obtained performances and the lab test, the realized sensor results suitable for the on-field monitoring of gas traces of methane, nitrous oxide and ammonia for agriculture and food production industry applications.

#### CRediT authorship contribution statement

**GM:** conceptualization, methodology, investigation, data curation, writing- Original draft. **AZ:** conceptualization, methodology, investigation, data curation, writing- Original draft. **EK:** Investigation, data curation; **SDR:** Investigation, data curation; **ACR:** Investigation, data curation; **ER:** methodology, data curation; **PP:** conceptualization, methodology, writing- Review & editing, funding acquisition; **AS:** conceptualization, methodology, writing- Review & editing; **MG:** methodology, investigation, data curation; **FM:** writing- Review & editing; **ED:** writing- Review & editing; **GP:** writing- Review & editing; **HW:** methodology, writing- Review & editing; **LD:** methodology, writing- Review & editing; **VS:** conceptualization, methodology, writing- Review & editing, Supervision.

#### Declaration of Competing Interest

The authors declare that they have no competing interests.

#### Data availability

Data will be made available on request.

#### Acknowledgments

The project was sponsored by the National Key R&D Program of China (No. 2019YFE0118200); the European Union's Horizon 2020 Research and Innovation Program under the Marie Skłodowska-Curie project OPTAPHI (grant No. 860808); the European Union's Horizon 2020 Research and Innovation Program under grant agreement (No. 101016956 PASSEPARTOUT); National Natural Science Foundation of China (NSFC) (Nos. 62175137, 62075119 and 61805132); Shanxi Science Fund for Distinguished Young Scholars (No. 20210302121003).

#### References

- [1] T.M. Letcher, Introduction with a focus on atmospheric carbon dioxide and climate change. Future Energy, Elsevier, Amsterdam, 2020, pp. 3–17, <https://doi.org/10.1016/B978-0-08-102886-5.00001-1>.
- [2] S. Das, W. Wang, S. Reeves, R.C. Dalal, Y.P. Dang, A. Gonzalez, P.M. Kopittke, Non-target impacts of pesticides on soil N transformations, abundances of nitrifying and denitrifying genes, and nitrous oxide emissions, *Sci. Total Environ.* 844 (2022), 157043, <https://doi.org/10.1016/j.scitotenv.2022.157043>.
- [3] IPCC, A.R.5 Synthesis report: climate change 2014. <https://www.ipcc.ch/report/ar5/syr/>, 2015 (accessed 2 August 2022).
- [4] F.N. Tubiello, M. Salvatore, A.F. Ferrara, J. House, S. Federici, S. Rossi, R. Biancalani, R.D.C. Golec, H. Jacobs, A. Flammini, P. Prosperi, P. Cardenas-Galindo, J. Schmidhuber, M.J.S. Sanchez, N. Srivastava, P. Smith, The contribution of agriculture, forestry and other land use activities to global warming, 1990–2012, *Glob. Change Biol.* 21 (7) (2015) 2655–2660, <https://doi.org/10.1111/gcb.12865>.
- [5] S.C. Vac, G.E. Popit, N. Frunzeti, A. Popovici, Evaluation of greenhouse gas emission from animal manure using the closed chamber method for gas fluxes, *Not. Bot. Horti Agrobot. Cluj.-Napoca* 41 (2013) 576–581, <https://doi.org/10.15835/nbha4129259>.
- [6] M. Li, C.J. Weschler, G. Beko, P. Wargocki, G. Lucic, J. Williams, Human ammonia emission rates under various indoor environmental conditions, *Environ. Sci. Technol.* 54 (2020) 5419–5428.
- [7] F.J. Dentener, P.J. Crutzen, A three-dimensional model of the global ammonia cycle, *J. Atmos. Chem.* 19 (1994) 331–369, <https://doi.org/10.1007/BF00694492>.
- [8] W.A.H. Asman, Factors influencing local dry deposition of gases with special reference to ammonia, *Atmos. Environ.* 32 (3) (1998) 415–421, [https://doi.org/10.1016/S1352-2310\(97\)00166-0](https://doi.org/10.1016/S1352-2310(97)00166-0).
- [9] G.H. Mount, B. Rumbur, J. Having, B. Lamb, H. Westberg, D. Yonge, K. Johnson, R. Kincaid, Measurement of atmospheric ammonia at a dairy using differential optical absorption spectroscopy in the mid-ultraviolet, *Atmos. Environ.* 36 (11) (2002) 1799–1810, [https://doi.org/10.1016/S1352-2310\(02\)00158-9](https://doi.org/10.1016/S1352-2310(02)00158-9).
- [10] J. Hodgkinson, R.P. Tatam, Optical gas sensing: a review, *Meas. Sci. Technol.* 24 (2013), 012004, <https://doi.org/10.1088/0957-0233/24/1/012004>.
- [11] W. Ren, W. Jiang, F.K. Tittel, Single-QCL-based absorption sensor for simultaneous trace-gas detection of CH<sub>4</sub> and N<sub>2</sub>O, *Appl. Phys. B* 117 (1) (2014) 245–251, <https://doi.org/10.1007/s00340-014-5828-8>.
- [12] L. Dong, F.K. Tittel, C. Li, N.P. Sanchez, H. Wu, C. Zheng, Y. Yu, A. Sampaolo, R. J. Griffin, Compact TDLAS based sensor design using interband cascade lasers for mid-IR trace gas sensing, *Opt. Express* 24 (6) (2016) A528–A535, <https://doi.org/10.1364/OE.24.00A528>.
- [13] T.I. Yacovitch, S.C. Herndon, J.R. Roscioli, C. Floerchinger, R.M. McGovern, M. Agnese, G. Pétron, J. Kofler, C. Sweeney, A. Karion, S.A. Conley, E.A. Kort, L. Nähle, M. Fischer, L. Hildebrandt, J. Koeth, J.B. McManus, D.D. Nelson, M. S. Zahniser, C.E. Kolb, Demonstration of an ethane spectrometer for methane source identification, *Environ. Sci. Technol.* 48 (14) (2014) 8028–8034, <https://doi.org/10.1021/es501475q>.
- [14] A. Elia, P.M. Lugarà, C. Di Franco, V. Spagnolo, Photoacoustic techniques for trace gas sensing based on semiconductor laser sources, *Sensors* 9 (2009) 9616–9628, <https://doi.org/10.3390/s91209616>.
- [15] A.A. Kosterev, Y.A. Bakhirkin, R.F. Curl, F.K. Tittel, Quartz-enhanced photoacoustic spectroscopy, *Opt. Lett.* 27 (2002) 1902–1904, <https://doi.org/10.1364/OL.27.001902>.
- [16] P. Patimisco, A. Sampaolo, L. Dong, F.K. Tittel, V. Spagnolo, Recent advances in quartz enhanced photoacoustic sensing, *Appl. Phys. Rev.* 5 (2018), 011106, <https://doi.org/10.1063/1.5013612>.
- [17] S. Viciani, M. Siciliani de Cumis, S. Borri, P. Patimisco, A. Sampaolo, G. Scamarcio, P. De Natale, F. D'Amato, V. Spagnolo, A quartz-enhanced photoacoustic sensor for H<sub>2</sub>S trace-gas detection at 2.6 μm, *Appl. Phys. B* 119 (2014) 21–27, <https://doi.org/10.1007/s00340-014-5991-y>.
- [18] P. Patimisco, A. Sampaolo, H. Zheng, L. Dong, F.K. Tittel, V. Spagnolo, Quartz-enhanced photoacoustic spectrophones exploiting custom tuning forks: a review, *Adv. Phys. X* 2 (2016) 169–187, <https://doi.org/10.1080/23746149.2016.1271285>.
- [19] S. Dello Russo, M. Giglio, A. Sampaolo, P. Patimisco, G. Menduni, H. Wu, L. Dong, V.M.N. Passaro, V. Spagnolo, Acoustic coupling between resonator tubes in quartz-



enhanced photoacoustic spectrophones employing a large prong spacing tuning fork, *Sensors* 19 (2019) 4109, <https://doi.org/10.3390/s19194109>.


- [20] G. Menduni, A. Sampaolo, P. Patimisco, M. Giglio, S. Dello Russo, A. Zifarelli, A. Elefante, P.Z. Wiczorek, T. Starecki, V.M.N. Passaro, F.K. Tittel, V. Spagnolo, Front-end amplifiers for tuning forks in quartz enhanced photoacoustic spectroscopy, *Appl. Sci.* 10 (8) (2020) 2947, <https://doi.org/10.3390/app10082947>.
- [21] M. Giglio, A. Elefante, P. Patimisco, A. Sampaolo, F. Sgobba, H. Rossmadl, V. Mackowiak, H. Wu, F.K. Tittel, L. Dong, V. Spagnolo, Quartz-enhanced photoacoustic sensor for ethylene detection implementing optimized custom tuning fork-based spectrophone, *Opt. Express* 27 (2019) 4271–4280, <https://doi.org/10.1364/OE.27.004271>.
- [22] P. Patimisco, A. Sampaolo, M. Giglio, S. Dello Russo, V. Mackowiak, H. Rossmadl, A. Cable, F.K. Tittel, V. Spagnolo, Tuning forks with optimized geometries for quartz-enhanced photoacoustic spectroscopy, *Opt. Express* 27 (2019) 1401–1415, <https://doi.org/10.1364/OE.27.001401>.
- [23] I.E. Gordon, L.S. Rothman, R.J. Hargreaves, R. Hashemi, E.V. Karlovets, F. M. Skinner, E.K. Conway, C. Hill, R.V. Kochanov, Y. Tan, P. Weislo, A.A. Finenko, K. Nelson, P.F. Bernath, M. Birk, V. Boudon, A. Campargue, K.V. Chance, A. Coustenis, B.J. Drouin, J.M. Flaud, R.R. Gamache, J.T. Hodges, D. Jacquemart, E.J. Mlawer, A.V. Nikitin, V.I. Perevalov, M. Rotger, J. Tennyson, G.C. Toon, H. Tran, V.G. Tyuterev, E.M. Adkins, A. Baker, A. Barbe, E. Canè, A.G. Császár, A. Dudaryonok, O. Egorov, A.J. Fleisher, H. Fleurbaey, A. Foltynowicz, T. Furtenbacher, J.J. Harrison, J.M. Hartmann, V.M. Horneman, X. Huang, T. Karman, J. Karns, S. Kass, I. Kleiner, V. Kofman, F. Kwabia-Tchana, N. Lavrentieva, T.J. Lee, D.A. Long, A.A. Lukashchanskaya, O.M. Lyulin, V. Y. Makhnev, W. Matt, S.T. Massie, M. Melosso, S.N. Mikhailenko, D. Mondelain, H. S.P. Müller, O.V. Naumenko, A. Perrin, O.L. Polyansky, E. Raddaoui, P.L. Raston, Z. D. Reed, M. Rey, C. Richard, R. Tóbiás, I. Sadiek, D.W. Schwenke, E. Starikova, K. Sung, F. Tamassia, S.A. Tashkun, J. Vander Auwera, I.A. Vasilenko, A.A. Viganin, G.L. Villanueva, B. Vispoel, G. Wagner, A. Yachmenev, S.N. Yurchenko, The HITRAN2020 molecular spectroscopic database, *J. Quant. Spectrosc. Radiat. Transf.* 277 (2022), 107949, <https://doi.org/10.1016/j.jqsrt.2021.107949>.
- [24] O. Vaittinen, M. Metsälä, S. Persijn, M. Vainio, L. Halonen, Adsorption of ammonia on treated stainless steel and polymer surfaces, *Appl. Phys. B* 115 (2014) 185–196, <https://doi.org/10.1007/s00340-013-5590-3>.
- [25] R.G. Shulman, B.P. Dailey, C.H. Townes, Molecular dipole moments and stark effects. III. Dipole moment determinations, *Phys. Rev.* 78 (1950) 145, <https://doi.org/10.1103/PhysRev.78.145>.
- [26] J. Henningsen, N. Melander, Sensitive measurement of adsorption dynamics with nonresonant gas phase photoacoustics, *Appl. Opt.* 36 (1997) 7037–7045, <https://doi.org/10.1364/AO.36.007037>.
- [27] A. Schmohl, A. Miklos, P. Hess, Effects of adsorption–desorption processes on the response time and accuracy of photoacoustic detection of ammonia, *Appl. Opt.* 40 (2001) 2571–2578, <https://doi.org/10.1364/ao.40.002571>.
- [28] United States Environmental Protection Agency, Inventory of U.S. Greenhouse Gas Emissions and Sinks: 1990–2018. <https://www.epa.gov/ghgemissions/inventory-us-greenhouse-gas-emissions-and-sinks-1990-2018>, 2020 (accessed 2 August 2022).



**Giansergio Menduni** received the M.S. degree (cum laude) in Electronic Engineering in 2017 from the Technical University of Bari. Since 2018, he is a Ph.D. student at the Electric and Information Engineering Department of Polytechnic of Bari. Since 2022, he is an Assistant Professor in Applied Physics at the Physics Department of Polytechnic of Bari. His research activity is focused on the development of gas sensors based on Quartz Enhanced Photoacoustic Spectroscopy



**Andrea Zifarelli** obtained his M.S. degree (cum laude) in Physics in 2018 from the University of Bari. From the same year, he is a Ph.D. student at the Physics Department of the University of Bari, developing his research work at PolySense Lab, joint-research laboratory between Technical University of Bari and THORLABS GmbH. Currently, his research activities are focused on the development of gas sensors based on Quartz-Enhanced Photoacoustic Spectroscopy for detection of gas mixtures and broadband absorbers, exploiting non-conventional laser sources



**Kniazeva Elena** obtained her bachelor's (2018) and master's (2020) degrees at ITMO University, Saint-Petersburg. Her bachelor's degree was in optical technologies and materials during which she developed a red phosphor to create LEDs which can emit warm white light. Her Master's degree was obtained in light-guided photonics (fiber optics) where she developed a fiber bending sensor based on tilted Fiber Bragg gratings, which worked in reflection mode. Right now, Elena is a Marie Skłodowska-Curie Early-Stage Researcher in the OPTAPHI double doctorate program. Her is carried out at University of Bari in Italy, and University of Montpellier in France.



**Stefano Dello Russo** obtained his M.S. degree (cum laude) in Physics in 2018 from the University of Bari. From the same year, he is a Ph.D. student at the Physics Department of the University of Bari, developing his research work at PolySense Lab, joint-research laboratory between Technical University of Bari and THORLABS GmbH. Currently, he is working as researcher at the Italian Space Agency.



**Ada Cristina Ranieri** received the M.S. degree (cum laude) in Environmental Engineering in 2019 from the Polytechnic of Bari. Since 2019, she is a Ph.D. student in engineering for technological innovation at the Uninettuno University and at Physic Department of the Technical University of Bari. His research activity is focused on the application of gas sensors based on Quartz Enhanced Photoacoustic Spectroscopy



**Ezio Ranieri** received the M.S. degree (cum laude) in Civil Engineering in 1990 from the University of Bari. Since 1994, he is a Ph.D. in Environmental Engineering at the Polytechnic of Milano. Since 2001, he is a Researcher and Aggregate Professor at the Polytechnic of Bari. Since 2018, he is an Associate Professor in Environmental and Sanitary Engineering at the University of Bari. Author of more than 100 papers, his research activity is focused on Environmental Monitoring



**Pietro Patimisco** obtained the Master degree in Physics (cum laude) in 2009 and the PhD Degree in Physics in 2013 from the University of Bari. Since 2018, he is Assistant professor at the Technical University of Bari. Dr. Patimisco's scientific activity addressed the study and applications of trace-gas sensors, such as quartz-enhanced photoacoustic spectroscopy and cavity enhanced absorption spectroscopy in the mid infrared and terahertz spectral region, leading to several publications.





**Angelo Sampaolo** obtained his Master degree in Physics in 2013 and the PhD Degree in Physics in 2017 from University of Bari. He was an associate researcher in the Laser Science Group at Rice University from 2014 to 2016 and associate researcher at Shanxi University since 2018. Since 2019, he is Assistant Professor at Polytechnic of Bari. His research activity has focused on the development of innovative techniques in trace gas sensing, based on Quartz-Enhanced Photoacoustic Spectroscopy and covering the full spectral range from near-IR to THz




**Giorgio Provolo** obtained the Ph.D. in Agricultural Engineering in 1990. From 2010 is Full Professor in Rural Buildings at University of Milan. Research activities have addressed the technical, managerial, and legislative constraints related to livestock farms. He studied in detail aspects of Agricultural Engineering related to housing facilities and the management of manure to improve the sustainability of intensive livestock farming



**Marilena Giglio** received the M.S. degree (cum laude) in Applied Physics in 2014, and the Ph.D. Degree in Physics in 2018 from the University of Bari. Since 2021, she is a Assistant Professor at the Physics Department of the Technical University of Bari. Her research activity is focused on the development of gas sensors based on Quartz-Enhanced Photoacoustic Spectroscopy and on the optical coupling of hollow-core waveguides with interband- and quantum-cascade lasers.



**Hongpeng Wu** received his Ph.D. degree in atomic and molecular physics from Shanxi University, China, in 2017. From September, 2015 to October, 2016, he studied as a joint Ph.D. student in the Electrical and Computer Engineering Department and Rice Quantum Institute, Rice University, Houston, USA. Currently he is a professor in the Institute of Laser Spectroscopy of Shanxi University. His research interests include gas sensors, photoacoustic spectroscopy, photothermal spectroscopy and laser spectroscopy techniques



**Fabrizio Manassero** received the M.S. degree in Environmental Engineering in 2000 from the Politecnico di Torino. Since 2001, he is working in Gas Analysis with ETG Risorse e Tecnologia srl, he has covered different role in company particularly in the training, sales and R&D. Since 2017, he is the R&D Manager and since 2021 is Sales Manager. His research activity is focused on the development of gas analyser with different technology FTIR, IMS and QEPAS



**Lei Dong** received his Ph.D. degree in optics from Shanxi University, China, in 2007. From June, 2008 to December, 2011, he worked as a post-doctoral fellow in the Electrical and Computer Engineering Department and Rice Quantum Institute, Rice University, Houston, USA. Currently he is a professor in the Institute of Laser Spectroscopy of Shanxi University. His research interests include optical sensors, trace gas detection, photoacoustic spectroscopy and laser spectroscopy



**Elio Dinuccio** is currently Associate Professor at the Department of Agriculture, Forest and Food Sciences - University of Turin. He received in 2007 the PhD degree at the University of Turin in Agricultural and Environmental Engineering. He has expertise in agriculture engineering with special regards to mineral and organic fertilizers spreaders, animal waste management concerning water, soil and atmospheric pollution, nutrients application and agricultural by products valorization. He has specific competences on particulate matter, ammonia, and greenhouse gas emission measurement, abatement strategies and manure treatment technologies, energy production from ligno-cellulosic by-products and energy crops



**Spagnolo Vincenzo** received the degree (summa cum laude) and the Ph.D., both in physics, from University of Bari. He works as Full Professor of Applied Physics at the Technical University of Bari. In 2019, he became Vice-Rector of the Technical University of Bari, deputy to Technology Transfer. Since 2017, he is the director of the joint-research lab Poly-Sense, created by THORLABS GmbH and Technical University of Bari, devoted to the development and implementation of novel gas sensing techniques and the realization of highly sensitive QEPAS trace-gas sensors